

**Title: Ex vivo coronary stent implantation evaluated with digital image correlation**

**Authors:** L. Horny<sup>1</sup>, H. Chlup<sup>1</sup>, R. Zitny<sup>1</sup>, T. Vonavkova<sup>1</sup>, J. Vesely<sup>1</sup>, P. Lanzer<sup>2</sup>

**Affiliations and addresses:**

<sup>1</sup>Faculty of Mechanical Engineering, Czech Technical University in Prague

Technicka 4, Prague, 166 07, Czech Republic

<sup>2</sup>Gesundheitszentrum Bitterfeld/Wolfen gGmbH

Friedrich-Ludwig-Jahn-Straße 2, Bitterfeld/Wolfen, D-06749, Germany

**Corresponding author:** Lukas Horny, Faculty of Mechanical Engineering, Czech Technical

University in Prague, Technicka 4, 166 07, Prague, Czech Republic, tel.: +420 22435 2690,

fax: +420 23332 2482, [lukas.horny@fs.cvut.cz](mailto:lukas.horny@fs.cvut.cz)

**Abstract:**

Intracoronary stenting (PCI) has become standard revascularization technique to reopen blocked arteries. Although significant progress in stenting technology and implantation techniques has been made a number of problems remain. Specifically, stent sizing and inflation pressures are still a matter of scientific debates. Despite a large number of biomechanical computational simulations experimental data are rare, likely due to technical difficulties to measure dilatation pressures and coronary dimensions in the same settings. Our study shows that valuable data can be obtained by employing digital image correlation for 3D strain measurement during stent inflation ex-vivo that can provide further insight into the stent–artery wall interactions.

**Keywords:**

Artery wall–stent interaction; coronary stent; digital image correlation; experimental implantation; strain.

## **Abstract/Introduction**

Intracoronary stenting (PCI) has become standard revascularization technique to reopen blocked arteries. Although significant progress in stenting technology and implantation techniques has been made a number of problems remain [1-6]. Specifically, stent sizing and inflation pressures are still a matter of scientific debates. Despite a large number of biomechanical computational simulations [3,7-10] experimental data are rare [3,4,6,11], likely due to technical difficulties to measure dilatation pressures and coronary dimensions in the same settings. Our study shows that valuable data can be obtained by employing digital image correlation for 3D strain measurement during stent inflation ex-vivo that can provide further insight into the stent–artery wall interactions.

## **Methods**

### *Stent and PCI equipment*

The balloon-expandable CoCr coronary stent Kaname<sup>TM</sup> (Terumo Corporation, Tokyo, Japan) with nominal diameter 3.5 mm, and length 15 mm (at pressure 0.9 MPa; and diameter 3.73 mm at 1.6 MPa) was used in this study. The stent was premounted on PCI dilatation catheter RX-2 (Terumo Corporation).

### *Sample*

The sample of the main branch of the left coronary artery was obtained from autopsy. The male donor was 40 years old and atherosclerotic lesions were presented inside the sample. The experiment was performed 70 hours post mortem.

### *Experiment*

The sample was mounted into the experimental setup (Fig. 1) with both ends cannulated to allow catheterization. Displacement measurement was based on 3D digital image correlation (DIC) conducted with commercial system Dantec Q-450 (Dantec Dynamics, Ulm, Germany).

DIC is non-contact optical method based on the stereoscopic principle which is becoming more popular especially within the strain measurement of geometrically nonuniform objects. The algorithm identifies material points on the object surface and the correlation between consecutive images allows material point tracking. Detailed description can be found in the literature [12-15, 18]. A random pattern is required for successful automatic evaluation. It was created by careful spraying the surface of the sample with acrylic lacquer (two different colors were used, white color was used to create the first layer and subsequently black dots were created with another spray; Fig. 1).

The artery was recorded with two digital cameras (NanoSens Mk III, Dantec Dynamics; 1MPx CCD chip; lens Sigma EX, 105 mm, 1:2.8 D Macro) during the balloon expansion (sampling rate 25 Hz). In fully expanded state, the object ROI approx. 18\*3 mm\*mm was projected onto 600\*300 px\*px (in each camera). RX2 manometer was recorded with another camera to obtain time course of change of the balloon distending pressure (pressure transducer connected with PC was not available at the time of experiment). The stent was deployed within manual pressurization up to 1.6 MPa which spanned approximately 42 seconds.

## **Results**

DIC revealed significant overloading of the artery by the expanded stent. The results are depicted in Figure 2. Principal strains' distribution (Green-Lagrange strain is considered within this study) shows artery response within maximally expanded stent. Principal vectors are predominantly aligned with the circumferential and longitudinal direction which is supposed to be the consequence of the cylindrical stent expansion.

Circumferential deformation attains 0.5 mm/mm at the peak value which is far beyond physiological situation. The circumferential strain concentration appears non-symmetrically with respect to the length of the sample which is supposed to be the result of irregular reference geometry (an asymmetrical partially occluded lumen of the artery). Fig. 2B shows areas of compressive longitudinal strain. This is in accordance with the simplified idea of dilated tubular structure inside a vessel (see Fig. 4).

Six points (P1-6) were chosen to illustrate specific strain values (Fig. 2). We also computed stresses at these points by direct substitution into the constitutive equation adopted from [16]. However, unrealistically high values were obtained and their presentation is omitted. It is probably due to unsuitable constitutive equation resulting from different loading conditions and atherosclerotic specimen in our experiment.

Figure 3 illustrates displacements observed on lines and points on the surface. Interestingly balloon pressure–displacement relationships (panel C) indicate that non-uniform and abrupt initial stent expansion (at approx. 0.18–0.3 MPa), reported in [3], might be detectable also on the object surface.

## **Discussion**

This is a preliminary report concerning a stent implantation in ex-vivo settings employing a human coronary artery harvested from autopsy. The results suggest that 3D DIC is promising tool suitable for the evaluation of ex-vivo stent implantation potentially useful for validation of computational models and clinical considerations.

Presented results suggest that overexpansion of a stent during deployment may overstretch the target site potentially resulting in implantation injury associated with restenosis and/or intimal tears associated with dissections.

To obtain exact intraluminal dimensions during stent deployment optical coherence tomography or intravascular ultrasound (IVUS) would be required, currently not available in our laboratory. Nevertheless we plan to combine IVUS with 3D DIC in future experiments.

## **Acknowledgement**

This work has been supported by Czech Ministry of Education, by Technology agency of the Czech Republic TA 01010185, by Czech Science Foundation P108/10/1296, and Grant Agency of the Czech Technical University in Prague SGS10/247/OHK2/3T/12.


## **References**

1. Lanzer P, Gijzen, FJH, Topoleski LDT, Holzapfel GA (2010) Call for Standards in Technical Documentation of Intracoronary Stents. *Herz* 35:27-33 doi: 10.1007/s00059-010-3278-6
2. Moore Jr. JE (2009) Biomechanical issues in endovascular device design. *J Endovasc Ther* 16(Suppl 1):I1-I11 doi: 10.1583/08-2605.1

3. Kiouisis DE, Wulff AR, Holzapfel GA (2009) Experimental studies and numerical analysis of the inflation and interaction of vascular balloon catheter-stent systems. *Ann Biomed Eng* 37:315-330 doi: 10.1007/s10439-008-9606-9
4. Simons JW, Dalal A, Shockey DA (2010) Load deformation behavior of Nitinol stents. *Exp Mech* 50:835-843 doi: 10.1007/s11340-010-9341-7
5. Mani G, Feldman MC, Patel D, Agrawal CM (2007) Coronary stents: materials perspective. *Biomaterials* 28:1689-1710 doi:10.1016/j.biomaterials.2006.11.042
6. Grenacher L, Rohde S, Gänger E, Deutsch J, Kauffmann GW, Richter GM (2006) In vitro comparison of self-expanding versus balloon-expandable stents in a human ex vivo model. *Cardiovasc Intervent Radiol* 29:249-254 doi: 10.1007/s00270-004-0295-y
7. Holzapfel GA, Stadler M, Gasser TC (2005) Changes in the mechanical environment of stenotic arteries during interaction with stents: Computational assessment of parametric stent designs. *J Biomech Eng* 127:166-180 doi: 10.1115/1.1835362
8. Pericevic I, Lally C, Toner D, Kelly DJ (2009) The influence of plaque composition on underlying arterial wall stress during stent expansion: The case for lesion-specific stents. *Med Eng Phys* 31:428-433 doi: 10.1016/j.medengphy.2008.11.005
9. Mortier P, Holzapfel GA, De Beule M, Van Loo D, Taeymans Y, Segers P, Verdonck P, Verheghe B (2010) A novel simulation strategy for stent insertion and deployment in curved coronary bifurcations: Comparison of three drug-eluting stents. *Ann Biomed Eng* 38:88-99 doi: 10.1007/s10439-009-9836-5
10. Gastaldi D, Morlacchi S, Nichetti R, Capelli C, Dubini G, Petrini L, Migliavacca F (2010) Modelling of the provisional side-branch stenting approach for the treatment of atherosclerotic coronary bifurcations: Effects of stent positioning. *Biomech Model Mechanobiol* 9:551-561 doi: 10.1007/s10237-010-0196-8
11. Takashima K, Kitou T, Mori K, Ikeuchi K (2007) Simulation and experimental observation of contact conditions between stents and artery models. *Med Eng Phys* 29:326-335 doi: 10.1016/j.medengphy.2006.04.003
12. Zhang D, Eggleton CD, Arola DD (2002) Evaluating the mechanical behavior of arterial tissue using digital image correlation. *Exp Mech* 42:409-416 doi: 10.1007/BF02412146
13. Sutton MA, Ke X, Lessner SM, Goldbach M, Yost M, Zhao F, Schreier HW (2008) Strain field measurements on mouse carotid arteries using microscopic three-dimensional digital image correlation. *J Biomedical Mater Res A* 84:178-190 doi: 10.1002/jbm.a.31268.


14. Becker T, Splitthof K, Siebert T, Kletting P. (2006) Error estimations of 3D digital image correlation measurements. *Proceedings of SPIE*, 6341:63410F doi: 10.1117/12.695277
15. Xu S, Grande-Allen KJ (2010) The evolution of the field of biomechanics through the lens of experimental mechanics. *Exp Mech* Volume 50:667-682 doi: 10.1007/s11340-010-9367-x
16. Holzapfel GA, Sommer G, Gasser CT, Regitnig P (2005) Determination of layer-specific mechanical properties of human coronary arteries with nonatherosclerotic intimal thickening and related constitutive modeling. *Am J Physiol* 289:H2048-H2058 doi: 10.1152/ajpheart.00934.2004
17. Freeman JW, Snowhill PB, Nosher JL (2010) A link between stent radial forces and vascular wall remodeling: The discovery of an optimal stent radial force for minimal vessel restenosis. *Connect Tissue Res* 51:314-326 doi: 10.3109/03008200903329771
18. Sutton MA, Orteu J-J, Schreier HW (2009) *Image Correlation for Shape, Motion and Deformation Measurements - Basic Concepts, Theory and Applications*. Springer Science+Business, New York

## Figure legends

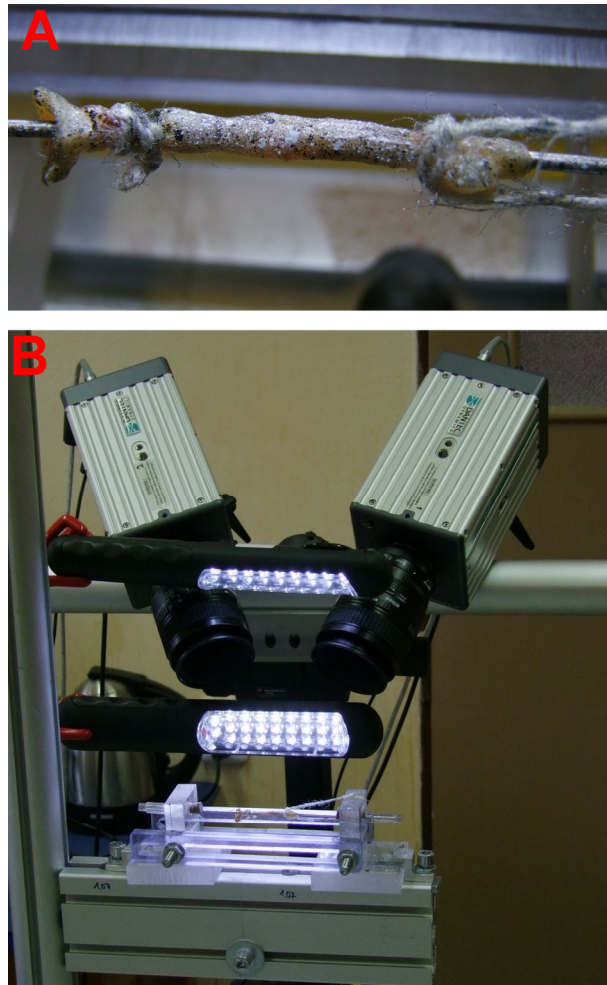


**Figure 1** A – the sample with random pattern on the surface. B – experimental setup.




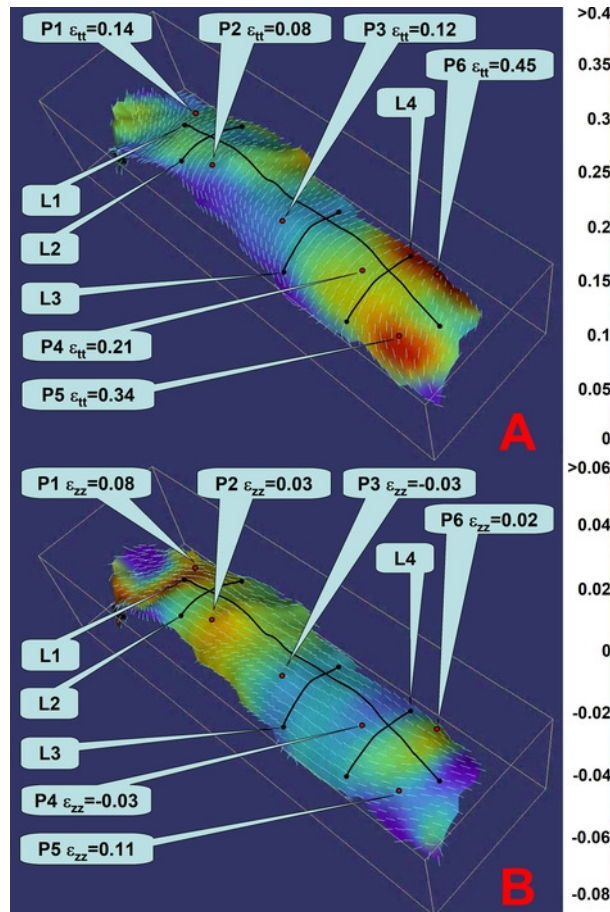

**Figure 2** Evaluated part of the artery surface after total stent expansion. A – color map of the first principal strain; B – second principal strain. The position of evaluated points (P1-6) and lines (L1-4) is depicted. Strains evaluated at P1-6 are denoted with indices “tt” and “zz” since they are considered to be parallel with circumferential and longitudinal strains in a pressurized vessel. It should be noted, however, that in case of “zz” tangential plane of the surface (where the strains are evaluated) may be deflected from longitudinal direction. Scale of the bars – Green-Lagrange strain [mm/mm]. The object is bounded by assistant lines oriented according to global Cartesian coordinate system (not scaled).

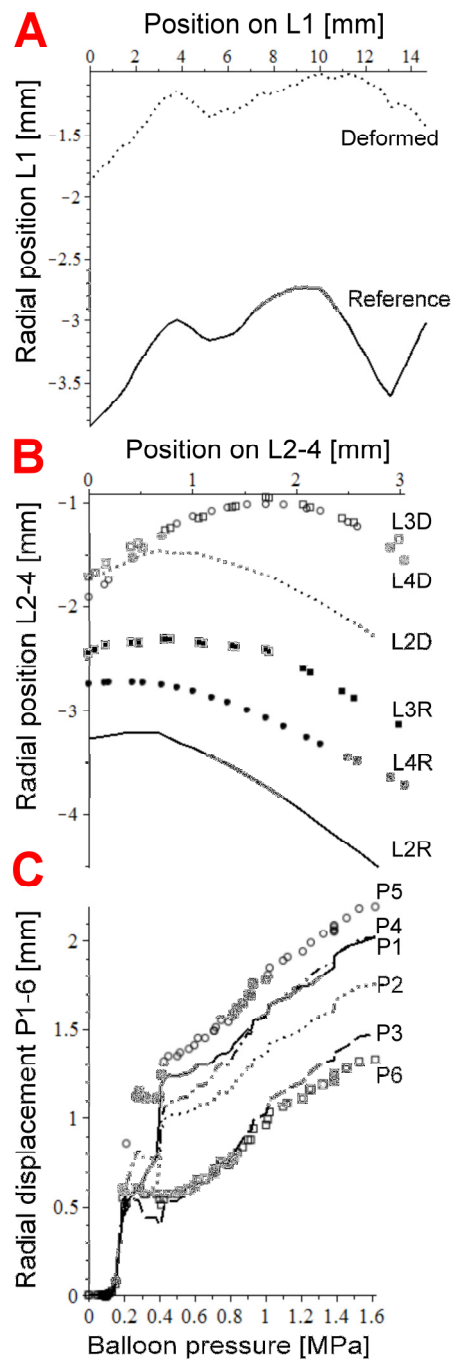

**Figure 3** Displacements and coordinates of entities on the object surface. A – reference and deformed coordinates of L1. B – coordinates of L2-4 (R = reference = non-expanded stent; D = deformed = totally expanded). C – displacements of P1-6 with respect to the pressure in the expansion balloon.

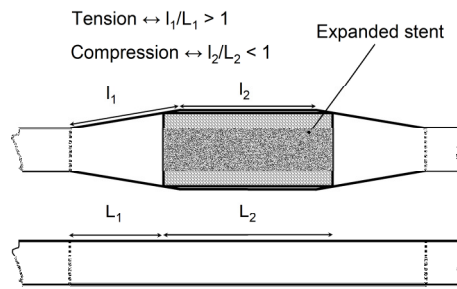

**Figure 4** Simplified model kinematics explaining compression of the object surface during stent expansion.